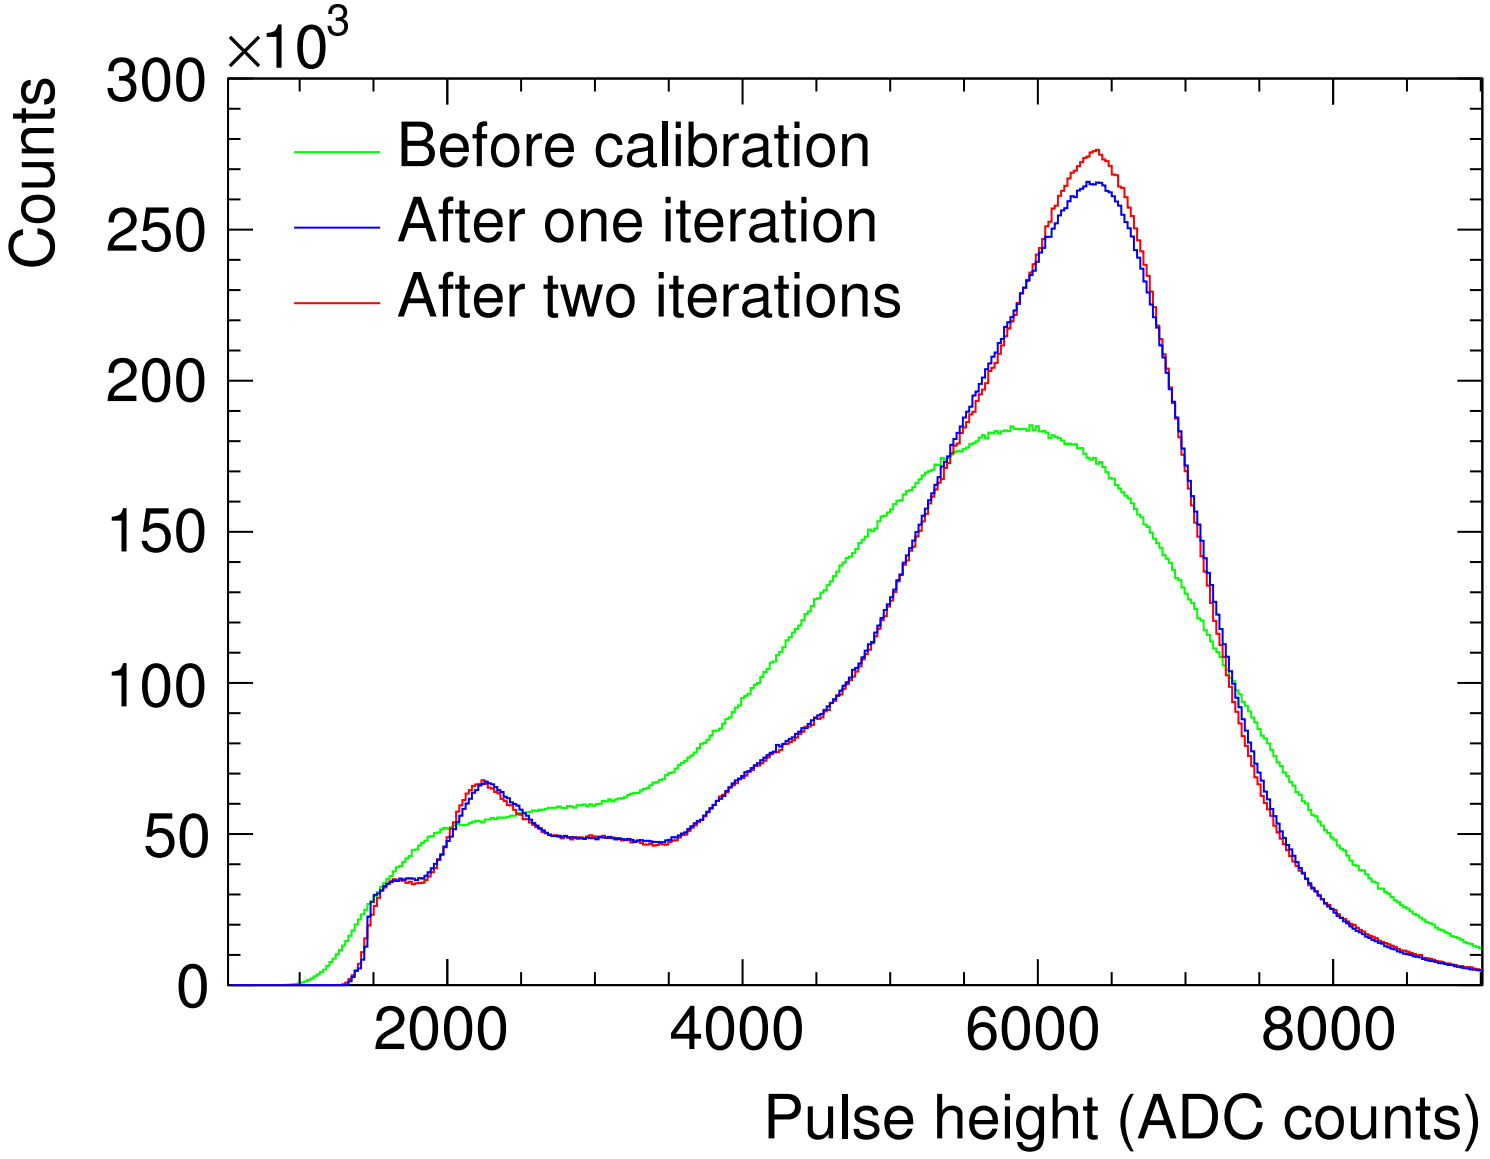
Counts
×10^3
300
250
200
150
100
50
0
Before calibration
After one iteration
After two iterations
2000
4000
6000
8000
Pulse height (ADC counts)